

## High Flow Oxygen Therapy – MaxVenturi®


## Guidance for Use\*

- 1. Select correct size of AquaNASE® nasal cannulae.
- 2. Apply AquaNASE® nasal cannulae and secure neck strap as shown overleaf.
- 3. Insert humidification chamber onto heater plate and spike water bag.
- 4. Attach circuit as shown a-d.

- 5. Connect heater cable and temperature probes.
- 6. Turn on heater and select invasive mode.
- Set flow at 20L/min and select prescribed FiO<sub>2</sub> for 2 minutes.



8. Increase flow to max 70L/min as required monitoring SpO<sub>2</sub> and respiratory rate.

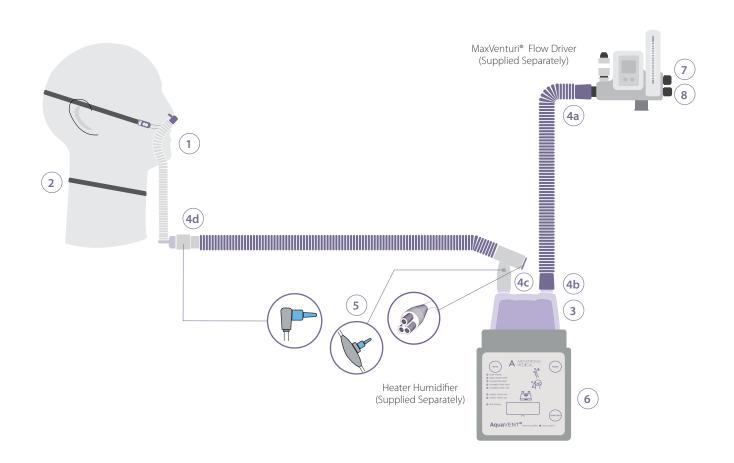

<sup>\*</sup>This guidance should be read in conjunction with the IFU supplied with the specific Breathing Circuit, Heater Humidifier, AquaNASE® nasal cannulae and the Flow Driver.

T +44 (0) 28 7035 6029 F +44 (0) 28 7035 6875

in fo@armstrong medical.net



## **AquaNASE**®

## Fitting Guide:

Step 1
Fit the looped neck
support strap by placing

support strap by placing over patients head and sliding down around the neck as shown.





Step 2 Adjust the looped neck support strap by pulling one strap through the

clamp as shown.





Step 3
Place the elasticated strap around the patients head.





Step 4
Adjust the ends of the elasticated strap to secure the device.





Armstrong Medical Wattstown Business Park, Newbridge Road, Coleraine, BT52 1BS, Northern Ireland. T +44 (0) 28 7035 6029 F +44 (0) 28 7035 6875

info@armstrongmedical.net



armstrongmedical.net

© Armstrong Medical Ltd. 2018